

Doci	ument Number: SASoM/METHOD/087.v3
Title:	MCM2 and Rabbit pan cytokeratin Immunofluorescence with Haematoxylin counterstain using Dako Link48
Version:	v3
Author:	In Hwa Um

Effective from:	15/03/20		
Valid to:	14/03/22		
Valia to:	14/00/22		

SOP History		
Number	Date	Reason for Change
v1	15/03/16	Original
v2	15/03/18	Update
v3	15/03/20	Biennial Update

1.0 Purpose -

This SOP describes the current procedure for staining cytology samples and formalin fixed paraffin embedded tissue sections with MCM2(Cytosystem) and Rabbit pan cytokeratin antibodies using Dako Link 48 in Laboratory 248 at the St Andrews School of Medicine (SASOM).

2.0 Scope -

This SOP applies to the staff in the SASoM involved with MCM2 + rabbit pan cytokeratin immunofluorescence with haematoxylin counterstain using Dako Link48.

3.0 Responsibilities -

All staff involved in IF using DAKO Link48 are responsible for ensuring that the methods are followed in accordance with this SOP. All staff must have read and signed the relevant risk assessment documents before performing this procedure.



4.0 Procedure -

MCM2+Rabbit pan-cytokeratin immunofluroscence in Dako Link48

- 1. Turn on Dako automation system UPS and computer.
- 2. Double-click the DakoLink icon on the computer desktop and log in.



DakoLink

3. Insert slide information in New slides tab


🙆 DakoLi	nk								
System Ad	ministration Help	_						_	
	New slides		Workflow	-	Instruments		Completed		
New	slides								
Patient	case								
Case numbe 4567	er:		Accession	number:	Hospital: Downtown Hos	pital 🗸			
First name:	Middle name:	Last name:	Accession	date:	Pathologist:	-			
John	L.	Doe	7/10/2013	2	V Dr. A	*			
Slides									
Protoco	al: elanosome HM845	Block:	Type:		eparation: D	rop zones:	Control si de	Silde notes:	Quantity:
3.1	Add Pa		ase inf				Counterstain		
3.2				-	ntibody	4MCI		(' whic	h includes ' IF
0.2			•				visualiza	•	
3.3	Block-								
3.4	Type-s	•							
3.5		•	hoose	eithei	FFPE	or Cvt	oloav		
3.6					entre for				Drop zones:
	appro	priate 2	zones '	for FF	PE	-			
3.7	Slide	iotes-if	neces	sary	•				
3.8	Quant	ity							
3.9	Print a	nd app	ly the s	slide la	abels				
3.10	-								
3.11	Stick t	ne labe	on the	e slide	es				
Put th	e slide	s) in no	on-met	tallic r	[.] ack. <u>(N</u>	<u>o dev</u>	vaxing a	nd reh	<u>ydration steps</u>
requir	<u>ed)</u>								
l anti	gen ret	rieval							
4.1 Ma	ake up E	EDTA-T	ris 1 L	solut	ion:				
			10m	M Tri	s Base =	= 1.21	g		

10mM Tris Base = 1.21g 1mM EDTA = 0.37g Tween = 0.5ml dH20 = 1L Add the EDTA and Tris Base to a 1L flask and add the dH20 and mix on magnetic stirrer. Ensure that the pH is 9. Add theTween.



- 4.2 Pour the antigen retrieval solution into the microwave pressure cooker. Screw on the lid and put into the microwave on high power to heat up for 13mins.
- 4.3 Perform antigen retrieval on slides by putting slide rack into pre-heated pressure cooker. Screw on the lid and place the red weight over the vent. Put back into the microwave and heat on high for 5mins there should be an audible hissing sound towards the end of the procedure.
- 4.3 Using heat resistant gloves and eye protection carefully lift the pressure cooker from within the microwave and place in sink. Place eye protection on. With the heat resistant gloves release the pressure by removing the weight from the top of the cooker. Stand well back immediately once the weight is removed. Do not stand over the pressure cooker during this step.
- 4.4 Allow the slides to cool down for 20mins. (<u>Do not add cold tap water into the pressure cooker</u>).

5. Monitor Workflow tab

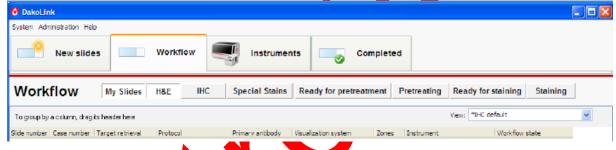

- 5.1 My slides tab will show the slides you entered.
- 5.2 Determine and prepare required reagents using DAKO reagent bottles by registering them with Lot number and expiry date (5ml, 12ml and 25ml).
 - 5.2.1 Endogenous enzyme block (Dako, #SM801) or equivalent to 3% H2O2 (Sigma, #H1009)
 - 5.2.2 Dako protein block (Dako, #X0909)
 - 5.2.3 Primary antibody- MCM2(Cytosystem, #03/0912, 1in500) + Rabbit pan-OK(Dako, #Z0622, 1in150)
 - Secondary reagent- anti-rabbit AF555 (Invitrogen, #A21428, 1in50) in anti-mouse HRP (Dako, #K4001)
 - 5.2.5 Tertiary reagent- TSA cy5(PerkinElmer, #NEL745B001KT) in amplification diluent (1in100)
 - 5.2.6 Counterstain- Harris Haematoxylin and Scotts tap water substitute
 - 2.7 Prepare wash buffer (DAKO, #DM831) or equivalent wash buffer (0.05% PBST) and deionised water and make sure waste bottle is
 - (0.05% PBST) and deionised water and make sure waste bottle empty.
- 5.3 Print and apply labels for each reagent's bottle and load it to the reagent rack and the rack to the machine.
- 6. Wash slides in wash buffer for 5min
- 7. Load slides into the black slide rack on the machine and moisten slides with wash buffer. (*Note:Make sure the slide rack is straight and even.)



8. Click the **'Instrument'** tab and choose 'AS1173D0903' Prime the buffer and water. When the following message displays, click OK. In this step, please make sure in the buffer and water nozzles are not having any air bubbles. If there's then repeat priming the buffer and water.

Autostainer Priming	
Autostainer	priming
Autostainer 1	
[Prime buffer Prime water Close
🛛 😑 will home and m	s prepared to prime the selected bulk fluid. The robot ove to the priming location. Press "Ok" to continue with "Cancel" to cancel priming. [214380]
(Note: <mark>Green</mark> co Yellow inc Conditions that o before the run ca <mark>Red</mark> indica	in the instruments tab lour indicates normal operation message dicates instrument needs attention but will not spoil slides. cause yellow alerts include indications that reagents are required an be processed. ates that you need to address the problem immediately. cause red alerts include system error messages.)
PTLinks	Autostainer 1
Artisan 1 Autostainer 1 Autostainer 2 Autostainer 2 Autostainer 2 Autostainer 2 A list of all stainers displays here.	Slides detected: 6. Research have been correctly placed. Total run time: 00:08, Buffer: 1.8L, Water: 1.0L. Start run? [214080]
	Preparing run (Run ID: 28) [212001]

- During the staining run, every 30mins keep checking the screen if there's yellow or red warnings. If so, fix the problems. Eg) Lack of reagents (yellow warning) – add more reagents)
- 11. End of the run, click the DONE button then the machine will purge the waste liquid.
- 12. Open the autostainer lid and remove completed slide racks and transfer each slide into designated wash buffer jar.
- 13. Dehydrate the slides in 80% alcohol for 1 min and air dry in the dark.
- 14. Mount slides with prolong gold anti-fade medium.



5.0 Troubleshooting

F	PDF	manual	is	availa	able	in	Help
							-

Help		
	Manuals	۲
	Safety notes	
	Request support	
	Registration	
	System information	
	Protocol PIN code	
	About Dako Link	

6.0 Personal protection -

A Howie laboratory coat and lab gloves must be worn at all times.

7.0 Spillages -

Always clean up any spills immediately after use, only you know what you have spilt and are aware of its hazard.

8.0 Training -

All staff should undergo training in this technique before performing procedure.

9.0 Related documents -

- 9.1 Risk assessments COSHN RA 08
 - General RA 06
- 9.2 SOP SASoM/EQUIP/015 Use of the Pressure Cooker for Antigen Retrieval



9.0 Approval and sign off -

Author:		
Name:	In Hwa Um	
Position:	Post Doc	
Signature:		Date:
Management Appr	oval:	
Name:	Peter Mullen	
Position:	Reseach Fellow	
Signature:		Date:
QA release by:		
Name:	Alex MacLellan	
Position:	QA Manager	
Signature:		Date:





STANDARD OPERATING PROCEDURE

Please sign below to indicate you have read this S.O.P and understand the procedures involved.

POSITION HELD	SIGNATURE	DATE
	POSITION HELD	POSITION HELD SIGNATURE I I